

HACTIV Total Conventional Hip Investigation

Note: This analysis compares the HACTIV femoral stem prosthesis with all other total conventional hip prostheses.

This prosthesis has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2026>.

Note: Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator. Procedures using prostheses with no recorded use in 2025 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Conventional Hip Replacement

The revision rate of the HACTIV total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 1: Revision Rates of Primary Total Conventional Hip Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
HACTIV	145	3402	17846	0.81 (0.69, 0.96)
Other Total Conventional Hip	19558	565258	3605628	0.54 (0.53, 0.55)
TOTAL	19703	568660	3623474	0.54 (0.54, 0.55)

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the HACTIV total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Conventional Hip Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs
HACTIV	2.5 (2.0, 3.1)	3.2 (2.6, 3.8)	3.5 (2.9, 4.2)	3.7 (3.1, 4.4)	4.1 (3.4, 4.8)	4.5 (3.8, 5.3)
Other Total Conventional Hip	1.7 (1.7, 1.8)	2.1 (2.1, 2.2)	2.5 (2.4, 2.5)	2.7 (2.7, 2.8)	3.0 (3.0, 3.1)	3.3 (3.2, 3.3)

CPR	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs
HACTIV	4.8 (4.1, 5.8)	5.3 (4.4, 6.3)	5.7 (4.7, 6.9)	6.3 (5.1, 7.8)	6.7 (5.3, 8.5)	6.7 (5.3, 8.5)
Other Total Conventional Hip	3.5 (3.5, 3.6)	3.8 (3.7, 3.9)	4.1 (4.0, 4.2)	4.4 (4.3, 4.4)	4.7 (4.6, 4.8)	5.1 (5.0, 5.2)

CPR	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs
HACTIV	6.7 (5.3, 8.5)					
Other Total Conventional Hip	5.4 (5.3, 5.5)	5.8 (5.7, 5.9)	6.2 (6.0, 6.3)	6.6 (6.5, 6.7)	6.9 (6.8, 7.1)	7.3 (7.1, 7.5)

CPR	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	24 Yrs	25 Yrs
HACTIV							
Other Total Conventional Hip	7.7 (7.5, 7.9)	8.0 (7.8, 8.2)	8.5 (8.3, 8.8)	9.0 (8.7, 9.4)	9.6 (9.1, 10.0)	9.6 (9.1, 10.1)	10.3 (9.4, 11.2)

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the HACTIV total conventional hip prosthesis is compared to all other total conventional hip prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Conventional Hip Replacement

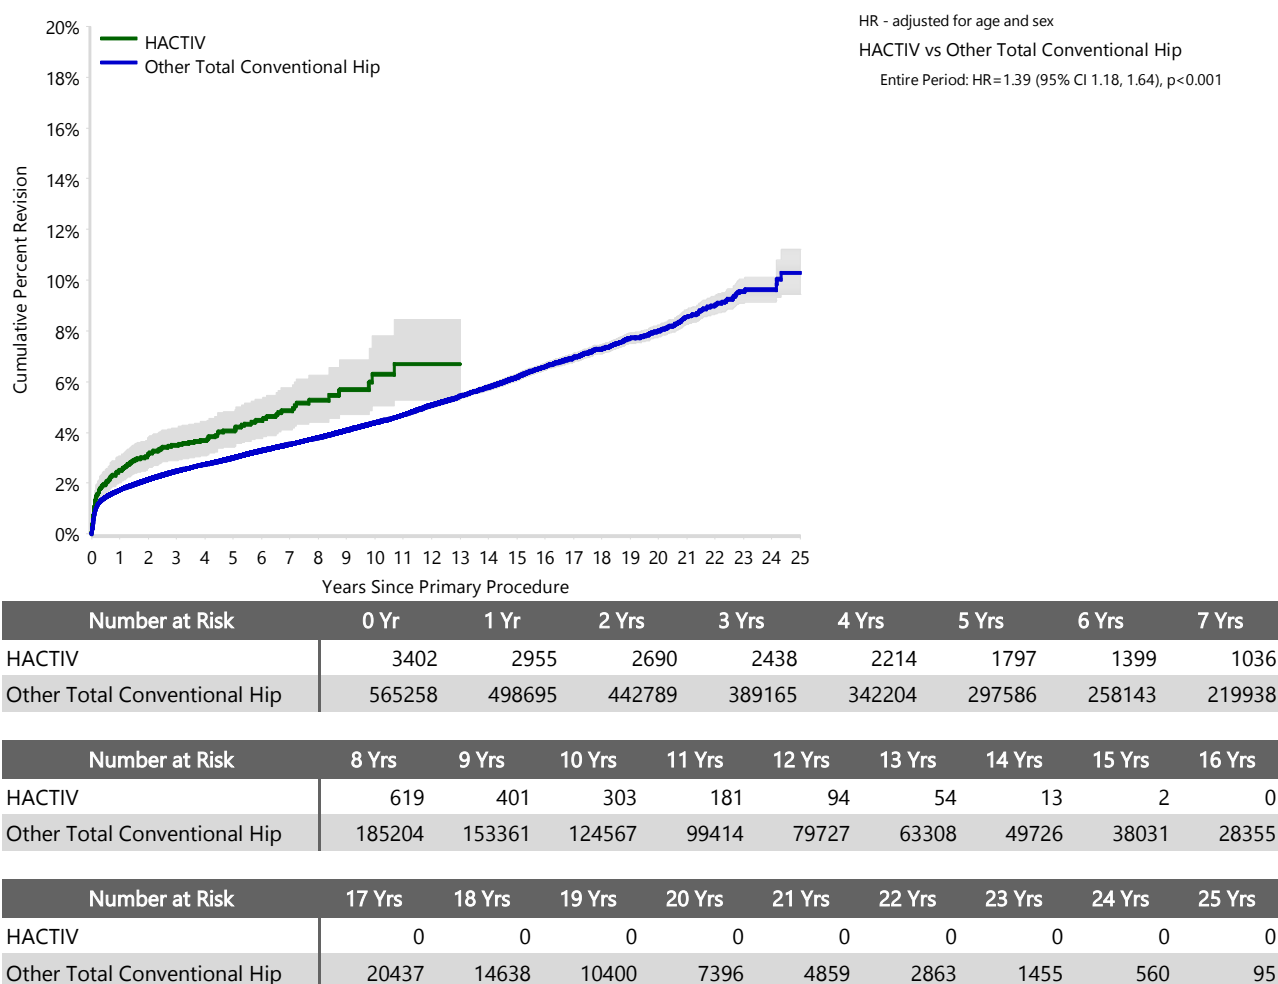

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Conventional Hip Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total conventional hip prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

Primary Diagnosis	HACTIV		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Osteoarthritis	137	94.5	16161	82.6
Fractured Neck Of Femur	1	0.7	1520	7.8
Osteonecrosis	2	1.4	842	4.3
Developmental Dysplasia	3	2.1	318	1.6
Rheumatoid Arthritis			201	1.0
Failed Internal Fixation			165	0.8
Tumour			157	0.8
Other Inflammatory Arthritis	1	0.7	101	0.5
Fracture/Dislocation			60	0.3
Other			21	0.1
Arthrodesis Takedown	1	0.7	12	0.1
TOTAL	145	100.0	19558	100.0

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Conventional Hip Replacement - Reason for Revision (Follow-up Limited to 15.1 Years)

Revision Diagnosis	Number	HACTIV		Other Total Conventional Hip		
		% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	33	1.0	22.8	4933	0.9	25.8
Prosthesis Dislocation/Instability	37	1.1	25.5	4290	0.8	22.4
Fracture	28	0.8	19.3	4211	0.7	22.0
Loosening	21	0.6	14.5	3496	0.6	18.3
Pain	5	0.1	3.4	330	0.1	1.7
Leg Length Discrepancy	2	0.1	1.4	305	0.1	1.6
Malposition	4	0.1	2.8	276	0.0	1.4
Implant Breakage Stem	1	0.0	0.7	197	0.0	1.0
Lysis	1	0.0	0.7	171	0.0	0.9
Implant Breakage Acetabular Insert	1	0.0	0.7	123	0.0	0.6
Incorrect Sizing	1	0.0	0.7	95	0.0	0.5
Wear Acetabular Insert				86	0.0	0.4
Metal Related Pathology	2	0.1	1.4	74	0.0	0.4
Implant Breakage Acetabular				70	0.0	0.4
Tumour				46	0.0	0.2
Wear Head				45	0.0	0.2
Heterotopic Bone				26	0.0	0.1
Implant Breakage Head				23	0.0	0.1
Wear Acetabulum				6	0.0	0.0
Osteonecrosis				4	0.0	0.0
Progression Of Disease				1	0.0	0.0
Synovitis	1	0.0	0.7	1	0.0	0.0
Other	8	0.2	5.5	312	0.1	1.6
N Revision	145	4.3	100.0	19121	3.4	100.0
N Primary	3402			565258		

Note: This table is restricted to revisions within 15.1 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Conventional Hip Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the HACTIV total conventional hip prosthesis. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total conventional hip prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Conventional Hip Replacement

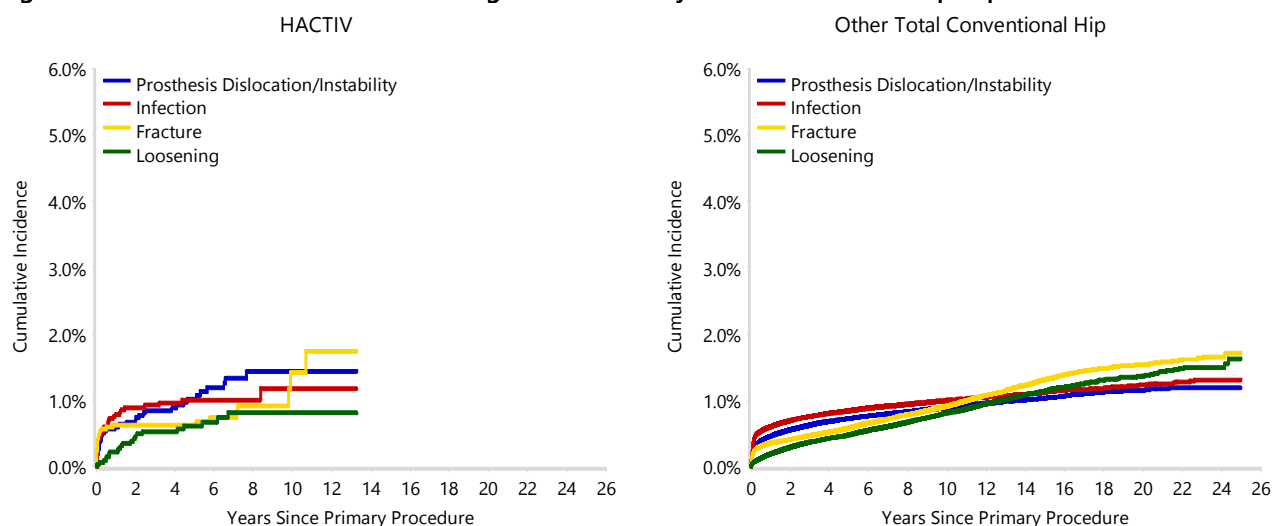


TABLE 5

Type of Revision Performed for Primary Total Conventional Hip Replacement

This analysis identifies the components used in the revision of the HACTIV total conventional hip prosthesis and compares it to the components used in the revision of all other total conventional hip prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total conventional hip prostheses i.e. is there a difference in the type of revision undertaken for the HACTIV total conventional hip prosthesis compared to all other total conventional hip prostheses.

Table 5: Primary Total Conventional Hip Replacement - Type of Revision (Follow-up Limited to 15.1 Years)

Type of Revision	HACTIV		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Femoral Component	35	24.1	6462	33.8
Acetabular Component	49	33.8	3165	16.6
THR (Femoral/Acetabular)	20	13.8	2196	11.5
Cement Spacer	5	3.4	549	2.9
Removal of Prostheses			91	0.5
Reinsertion of Components			27	0.1
Total Femoral			12	0.1
Bipolar Head and Femoral			10	0.1
N Major	109	75.2	12512	65.4
Head/Insert	32	22.1	5261	27.5
Head Only	4	2.8	900	4.7
Minor Components			279	1.5
Insert Only			166	0.9
Bipolar Only			1	0.0
Cement Only			1	0.0
Head/Neck/Insert			1	0.0
N Minor	36	24.8	6609	34.6
TOTAL	145	100.0	19121	100.0

Note: This table is restricted to revisions within 15.1 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 6**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Fixation

Fixation	N Revised	N Total
Cementless	144	3398
Hybrid (Femur Cemented)	1	3
Reverse Hybrid (Femur Cementless)	0	1
TOTAL	145	3402

TABLE 7**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this prosthesis are listed.

Table 7: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Ceramic/Ceramic	19	370
Ceramic/Non XLPE	24	1204
Ceramic/XLPE	79	1338
Ceramic/XLPE + Antioxidant	9	250
Metal/Non XLPE	9	131
Metal/XLPE	5	102
Metal/XLPE + Antioxidant	0	7
TOTAL	145	3402

TABLE 8**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Approach**

This analysis is provided as some prostheses are used with a variety of surgical approaches. All surgical approaches used with this prosthesis are listed.

Table 8: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Approach

Approach	N Revised	N Total
Anterior	18	440
Lateral	15	375
Posterior	92	2299
TOTAL	125	3114

Note: Excludes 288 procedures with no approach recorded

TABLE 9

Revision Rates of Primary Total Conventional Hip Replacement by State

This enables a state by state variation to be identified for the HACTIV total conventional hip prosthesis and provides the comparative data for each of the states for all other total conventional hip prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 9: Revised Number of Primary Total Conventional Hip Replacement by State

Component	State	N Revised	N Total
HACTIV	NSW	36	674
	VIC	0	4
	QLD	1	14
	WA	87	2405
	SA	20	299
	ACT/NT	1	6
Other Total Conventional Hip	NSW	5471	166349
	VIC	4853	146554
	QLD	3967	104345
	WA	2424	62559
	SA	1868	51793
	TAS	439	18269
	ACT/NT	536	15389
TOTAL		19703	568660

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 10**Number of Revisions of HACTIV Primary Total Conventional Hip Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the HACTIV total conventional hip prosthesis. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2025 has a maximum of one year to be revised, whereas a primary procedure performed in 2023 has a maximum of three years to be revised.

Table 10: Number of Revisions of HACTIV Primary Total Conventional Hip Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2010	0	2
2011	4	19
2012	1	63
2013	4	61
2014	10	117
2015	3	146
2016	1	96
2017	17	240
2018	25	452
2019	27	388
2020	20	418
2021	15	406
2022	3	194
2023	8	225
2024	2	225
2025	5	350
TOTAL	145	3402

TABLE 11

Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular HACTIV prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Material	Coating
Femoral Stem					
HACTIV	H49007-H49020	HA FEMORAL STEM	NO	METAL	HA COATED
HACTIV	H49C009-H49C020	HACTIV NON CEMENTED HAC COLLARED STEM	NO	METAL	HA COATED
HACTIV	H49L009-H49L020	HA LATERAL FEMORAL STEM	NO	METAL	HA COATED
HACTIV	H49LC009-H49LC020	FEMORAL STEM HIGH OFFSET COLLARED	NO	METAL	HA COATED

Table 11: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Catalogue Number Range

Femoral Stem Range	N Revised	N Total
H49007-H49020	35	840
H49C009-H49C020	45	1050
H49L009-H49L020	24	606
H49LC009-H49LC020	41	906
TOTAL	145	3402

TABLE 12**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Component**

A prosthesis may be combined with multiple components. This analysis has been undertaken to determine if the revision rate varies according to the component with which it is combined.

Table 12: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Acetabular Component

Acetabular Component	N Revised	N Total
Austral	4	71
Cer-Met	1	12
Delta-TT	9	130
FMP	0	13
Fin II	1	41
Furlong	1	18
G7	0	1
Logical G	84	1415
Marathon	0	1
PINNACLE	1	9
R3	0	5
Saturne	37	1461
Trabecular Metal (Shell)	0	2
Trident (Shell)	1	1
Trident/Tritanium (Shell)	0	14
Trinity	6	208
TOTAL	145	3402