Optetrak-PS/Optetrak Total Knee Investigation

Note: This analysis compares the Optetrak-PS/Optetrak femoral/tibial combination with all other total knee prostheses.

This combination has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, https://aoanjrr.sahmri.com/annual-reports-2026.

Note: Procedures using prostheses with no recorded use in 2025 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Knee Replacement

The revision rate of the Optetrak-PS/Optetrak total knee combination is compared to all other total knee prostheses.

Table 1: Revision Rates of Primary Total Knee Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
Optetrak-PS/Optetrak	425	2410	30127	1.41 (1.28, 1.55)
Other Total Knee	27284	791430	5145922	0.53 (0.52, 0.54)
TOTAL	**27709**	**793840**	**5176049**	**0.54 (0.53, 0.54)**

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Optetrak-PS/Optetrak total knee combination is compared to all other total knee prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Knee Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs
Optetrak-PS/Optetrak	1.5 (1.1, 2.0)	3.4 (2.8, 4.2)	4.8 (4.0, 5.7)	5.7 (4.9, 6.8)	6.4 (5.5, 7.5)	7.3 (6.4, 8.5)
Other Total Knee	1.0 (1.0, 1.0)	1.8 (1.8, 1.8)	2.4 (2.3, 2.4)	2.8 (2.7, 2.8)	3.1 (3.1, 3.1)	3.4 (3.4, 3.5)

CPR	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs
Optetrak-PS/Optetrak	8.5 (7.5, 9.8)	9.4 (8.3, 10.7)	11.0 (9.7, 12.3)	12.2 (10.9, 13.6)	14.0 (12.6, 15.6)	15.5 (14.0, 17.1)
Other Total Knee	3.7 (3.7, 3.8)	4.0 (4.0, 4.1)	4.3 (4.3, 4.4)	4.6 (4.6, 4.7)	4.9 (4.9, 5.0)	5.3 (5.2, 5.3)

CPR	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs
Optetrak-PS/Optetrak	18.0 (16.3, 19.7)	19.1 (17.4, 20.9)	20.1 (18.3, 22.0)	21.0 (19.2, 23.0)	22.2 (20.2, 24.2)	23.0 (20.9, 25.2)
Other Total Knee	5.6 (5.5, 5.7)	5.9 (5.8, 6.0)	6.3 (6.2, 6.4)	6.7 (6.6, 6.9)	7.2 (7.0, 7.3)	7.5 (7.4, 7.7)

CPR	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	24 Yrs	25 Yrs
Optetrak-PS/Optetrak	23.3 (21.3, 25.6)	23.6 (21.5, 26.0)	23.6 (21.5, 26.0)	23.6 (21.5, 26.0)			
Other Total Knee	7.9 (7.7, 8.0)	8.1 (7.9, 8.3)	8.5 (8.2, 8.7)	8.7 (8.4, 9.0)	8.8 (8.6, 9.2)	9.1 (8.7, 9.5)	9.5 (8.8, 10.2)

Note: Prostheses no longer used in 2025 are excluded from the comparator.

FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Optetrak-PS/Optetrak total knee combination is compared to all other total knee prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Knee Replacement

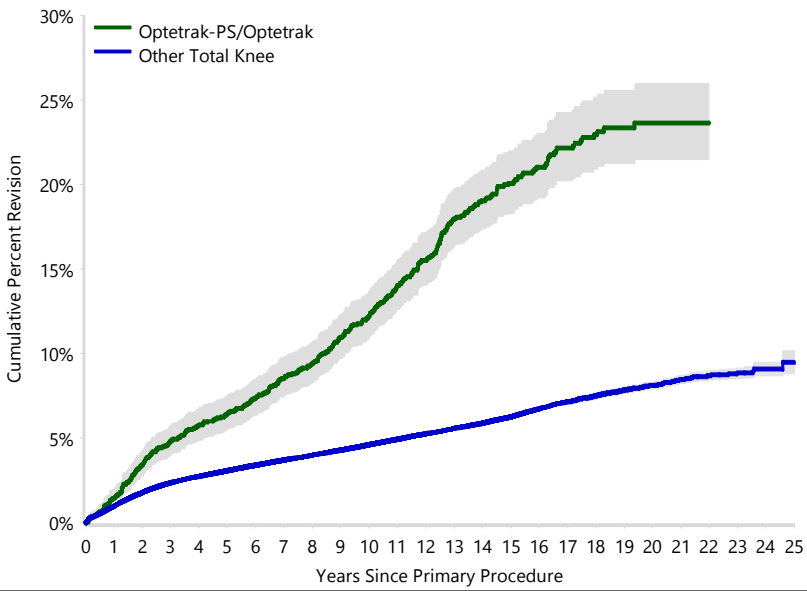

HR - adjusted for age and sex

Optetrak-PS/Optetrak vs Other Total Knee

0 - 1Mth: HR=0.22 (95% CI 0.03, 1.56), p=0.130

1Mth - 1.5Yr: HR=1.90 (95% CI 1.47, 2.47), p<0.001

1.5Yr - 2.5Yr: HR=2.83 (95% CI 2.11, 3.80), p<0.001

2.5Yr - 3Yr: HR=1.93 (95% CI 1.07, 3.50), p=0.029

3Yr - 5.5Yr: HR=2.27 (95% CI 1.69, 3.04), p<0.001

5.5Yr+: HR=4.44 (95% CI 3.93, 5.02), p<0.001

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs
Optetrak-PS/Optetrak	2410	2352	2288	2226	2168	2103	2036	1951
Other Total Knee	791430	708699	628274	550835	487544	424868	369845	315999

Number at Risk	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
Optetrak-PS/Optetrak	1877	1780	1693	1583	1413	1205	1027	838	680
Other Total Knee	266816	222320	182654	146980	117201	92187	70380	52526	38351

Number at Risk	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	24 Yrs	25 Yrs
Optetrak-PS/Optetrak	537	424	312	213	120	62	30	12	7
Other Total Knee	27628	19434	13616	9427	6164	3657	2096	972	244

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 3

Primary Diagnosis for Revised Primary Total Knee Replacement

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total knee prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Knee Replacement

	Optetrak-PS/Optetrak		Other Total Knee	
Primary Diagnosis	Number	Percent	Number	Percent
Osteoarthritis	415	97.6	26392	96.7
Rheumatoid Arthritis	10	2.4	330	1.2
Tumour			199	0.7
Other Inflammatory Arthritis			177	0.6
Osteonecrosis			104	0.4
Fracture			55	0.2
Other			26	0.1
Chondrocalcinosis			1	0.0
TOTAL	**425**	**100.0**	**27284**	**100.0**

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Knee Replacement - Reason for Revision

Revision Diagnosis	Optetrak-PS/Optetrak			Other Total Knee		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	60	2.5	14.1	7891	1.0	28.9
Loosening	158	6.6	37.2	5770	0.7	21.1
Instability	15	0.6	3.5	2873	0.4	10.5
Patella Erosion	8	0.3	1.9	2038	0.3	7.5
Pain	30	1.2	7.1	1867	0.2	6.8
Patellofemoral Pain	22	0.9	5.2	1557	0.2	5.7
Arthrofibrosis	5	0.2	1.2	1181	0.1	4.3
Fracture	12	0.5	2.8	1139	0.1	4.2
Malalignment	4	0.2	0.9	511	0.1	1.9
Wear Tibial Insert	16	0.7	3.8	374	0.0	1.4
Lysis	65	2.7	15.3	291	0.0	1.1
Implant Breakage Tibial Insert	6	0.2	1.4	252	0.0	0.9
Incorrect Sizing	2	0.1	0.5	218	0.0	0.8
Patella Maltracking	6	0.2	1.4	192	0.0	0.7
Bearing Dislocation				151	0.0	0.6
Implant Breakage Patella	5	0.2	1.2	147	0.0	0.5
Metal Related Pathology	1	0.0	0.2	114	0.0	0.4
Prosthesis Dislocation				78	0.0	0.3
Synovitis				64	0.0	0.2
Wear Patella	6	0.2	1.4	52	0.0	0.2
Osteonecrosis				51	0.0	0.2
Implant Breakage Femoral				49	0.0	0.2
Implant Breakage Tibial	3	0.1	0.7	39	0.0	0.1
Tumour				36	0.0	0.1
Heterotopic Bone				16	0.0	0.1
Progression Of Disease				8	0.0	0.0
Wear Tibial				6	0.0	0.0
Patella Dislocation				3	0.0	0.0
Incorrect Side				1	0.0	0.0
Wear Femoral				1	0.0	0.0
Other	1	0.0	0.2	314	0.0	1.2
N Revision	**425**	**17.6**	**100.0**	**27284**	**3.4**	**100.0**
N Primary	**2410**			**791430**		

Note: Prostheses no longer used in 2025 are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Knee Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the Optetrak-PS/Optetrak total knee combination. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total knee prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Knee Replacement

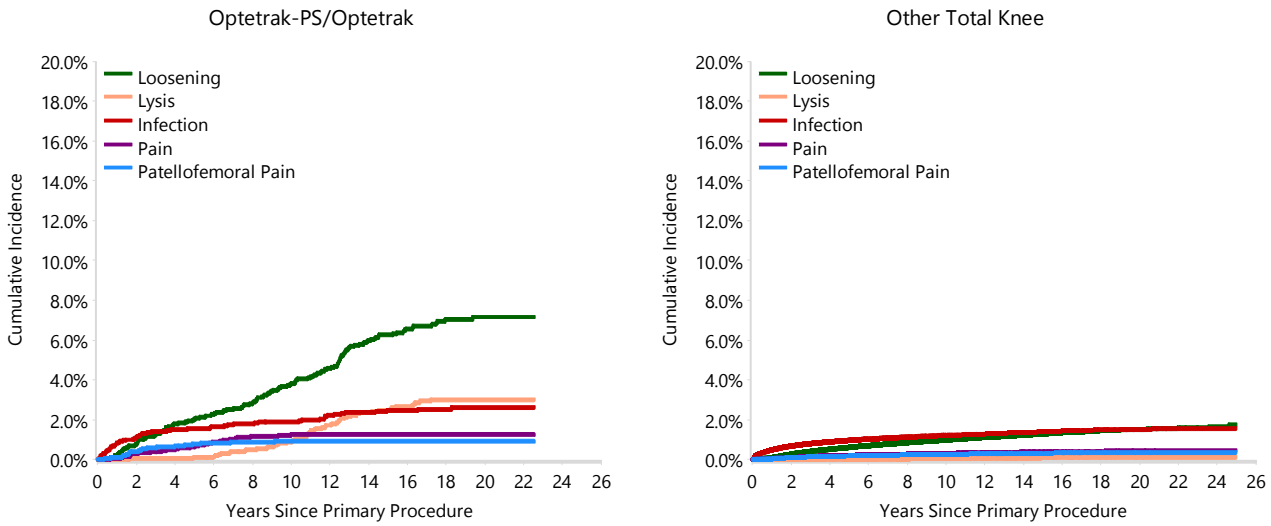

TABLE 5

Type of Revision Performed for Primary Total Knee Replacement

This analysis identifies the components used in the revision of the Optetrak-PS/Optetrak total knee combination and compares it to the components used in the revision of all other total knee prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total knee prostheses i.e. is there a difference in the type of revision undertaken for the Optetrak-PS/Optetrak total knee combination compared to all other total knee prostheses.

Table 5: Primary Total Knee Replacement - Type of Revision

	Optetrak-PS/Optetrak		Other Total Knee	
Type of Revision	Number	Percent	Number	Percent
TKR (Tibial/Femoral)	228	53.6	6673	24.5
Tibial Component	31	7.3	1908	7.0
Femoral Component	11	2.6	1313	4.8
Cement Spacer	13	3.1	1137	4.2
Removal of Prostheses	2	0.5	135	0.5
Total Femoral			23	0.1
Reinsertion of Components	1	0.2	8	0.0
N Major	**286**	**67.3**	**11197**	**41.0**
Insert Only	38	8.9	8575	31.4
Patella Only	53	12.5	4495	16.5
Insert/Patella	46	10.8	2940	10.8
Minor Components	1	0.2	66	0.2
Cement Only	1	0.2	11	0.0
N Minor	**139**	**32.7**	**16087**	**59.0**
TOTAL	**425**	**100.0**	**27284**	**100.0**

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 6

Revision Rates of Optetrak-PS/Optetrak Primary Total Knee Replacement by Fixation

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of Optetrak-PS/Optetrak Primary Total Knee Replacement by Fixation

Fixation	N Revised	N Total
Cemented	400	2236
Hybrid (Tibial Cemented)	25	174
TOTAL	**425**	**2410**

TABLE 7

Revision Rates of Optetrak-PS/Optetrak Primary Total Knee Replacement by Bearing Surface

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this combination are listed.

Table 7: Revised Number of Optetrak-PS/Optetrak Primary Total Knee Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Non XLPE	425	2410
TOTAL	**425**	**2410**

TABLE 8

Revision Rates of Optetrak-PS/Optetrak Primary Total Knee Replacement by Bearing Mobility

This analysis is provided as some prostheses are combined with a variety of bearing mobilities. All bearing mobilities used with this combination are listed.

Table 8: Revised Number of Optetrak-PS/Optetrak Primary Total Knee Replacement by Bearing Mobility

Bearing Mobility	N Revised	N Total
Fixed	425	2410
TOTAL	**425**	**2410**

TABLE 9

Revision Rates of Optetrak-PS/Optetrak Primary Total Knee Replacement by Stability

This analysis is provided as some prostheses are combined with a variety of stabilities. All stabilities used with this combination are listed.

Table 9: Revised Number of Optetrak-PS/Optetrak Primary Total Knee Replacement by Stability

Stability	N Revised	N Total
Fully Stabilised	1	1
Posterior Stabilised	424	2409
TOTAL	**425**	**2410**

TABLE 10

Revision Rates of Primary Total Knee Replacement by State

This enables a state by state variation to be identified for the Optetrak-PS/Optetrak total knee combination and provides the comparative data for each of the states for all other total knee prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 10: Revised Number of Primary Total Knee Replacement by State

Component	State	N Revised	N Total
Optetrak-PS/Optetrak	NSW	8	55
	VIC	5	48
	QLD	400	2246
	WA	12	56
	SA	0	3
	ACT/NT	0	2
Other Total Knee	NSW	7550	259497
	VIC	6020	163565
	QLD	5789	167244
	WA	3600	92841
	SA	3220	73114
	TAS	475	15075
	ACT/NT	630	20094
TOTAL		**27709**	**793840**

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 11

Number of Revisions of Optetrak-PS/Optetrak Primary Total Knee Replacement by Year of Implant

This analysis details the number of prostheses reported each year to the Registry for the Optetrak-PS/Optetrak total knee combination. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2025 has a maximum of one year to be revised, whereas a primary procedure performed in 2023 has a maximum of three years to be revised.

Table 11: Number of Revisions of Optetrak-PS/Optetrak Primary Total Knee Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2000	2	14
2001	3	22
2002	9	90
2003	16	130
2004	23	155
2005	32	252
2006	44	253
2007	34	216
2008	17	168
2009	39	202
2010	33	198
2011	52	202
2012	57	200
2013	35	151
2014	18	115
2015	7	30
2016	1	3
2017	3	5
2018	0	3
2019	0	1
TOTAL	**425**	**2410**

TABLE 12

Revision Rates of Optetrak-PS/Optetrak Primary Total Knee Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular Optetrak-PS/Optetrak prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Fixation
Femoral				
Optetrak-PS	2040101-2040106	PS CEMENTED FEMORAL COMPONENT	YES	
Optetrak-PS	2060101-2060106	PS POROUS FEMORAL COMPONENT	NO	POROUS
Optetrak-PS	2340200-2340306	PS CEMENTED ASYMMETRIC FEMORAL COMPONENT	YES	
Optetrak-PS	2440200-2440305	PS CEMENTED HI FLEX FEMORAL COMPONENT	YES	
Optetrak-PS	2460200-2460305	PS POROUS HI FLEX FEMORAL COMPONENT	NO	POROUS
Tibial				
Optetrak	2000421-2000612	CEMENTED FINNED TIBIAL TRAY	YES	
Optetrak	2040421-2040612	CEMENTED TRAPEZOID TIBIAL TRAY	YES	
Optetrak	2080411-2080454	CEMENTED OFFSET TIBIAL TRAY W/SCREW	YES	

Table 12: Revised Number of Optetrak-PS/Optetrak Primary Total Knee Replacement by Catalogue Number Range

Femoral Range	Tibial Range	N Revised	N Total
2040101-2040106	2000421-2000612	53	414
	2040421-2040612	16	94
2060101-2060106	2000421-2000612	20	132
	2040421-2040612	1	6
2340200-2340306	2000421-2000612	36	184
	2040421-2040612	155	862
2440200-2440305	2000421-2000612	17	94
	2040421-2040612	123	584
	2080411-2080454	0	1
2460200-2460305	2000421-2000612	3	19
	2040421-2040612	1	20
TOTAL		**425**	**2410**