CORAIL/Trabecular Metal (Shell) Total Conventional Hip Investigation

Note: This analysis compares the CORAIL/Trabecular Metal (Shell) femoral stem/acetabular combination with all other total conventional hip prostheses.

This combination has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, https://aoanjrr.sahmri.com/annual-reports-2026.

Note: Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator. Procedures using prostheses with no recorded use in 2025 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Conventional Hip Replacement

The revision rate of the CORAIL/Trabecular Metal (Shell) total conventional hip combination is compared to all other total conventional hip prostheses.

Table 1: Revision Rates of Primary Total Conventional Hip Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
CORAIL/Trabecular Metal (Shell)	11	100	917	1.20 (0.60, 2.15)
Other Total Conventional Hip	19690	568512	3622154	0.54 (0.54, 0.55)
TOTAL	**19701**	**568612**	**3623071**	**0.54 (0.54, 0.55)**

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the CORAIL/Trabecular Metal (Shell) total conventional hip combination is compared to all other total conventional hip prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Conventional Hip Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs
CORAIL/Trabecular Metal (Shell)	6.0 (2.8, 13.0)	8.2 (4.2, 15.8)	9.4 (5.0, 17.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)
Other Total Conventional Hip	1.7 (1.7, 1.8)	2.1 (2.1, 2.2)	2.5 (2.4, 2.5)	2.7 (2.7, 2.8)	3.0 (3.0, 3.1)	3.3 (3.2, 3.3)

CPR	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs
CORAIL/Trabecular Metal (Shell)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)
Other Total Conventional Hip	3.5 (3.5, 3.6)	3.8 (3.7, 3.9)	4.1 (4.0, 4.2)	4.4 (4.3, 4.5)	4.7 (4.6, 4.8)	5.1 (5.0, 5.2)

CPR	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs
CORAIL/Trabecular Metal (Shell)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)	11.8 (6.7, 20.3)			
Other Total Conventional Hip	5.4 (5.3, 5.5)	5.8 (5.7, 5.9)	6.2 (6.1, 6.3)	6.6 (6.5, 6.7)	7.0 (6.8, 7.1)	7.3 (7.1, 7.5)

CPR	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	24 Yrs	25 Yrs
CORAIL/Trabecular Metal (Shell)							
Other Total Conventional Hip	7.7 (7.5, 7.9)	8.0 (7.8, 8.2)	8.6 (8.3, 8.9)	9.0 (8.7, 9.4)	9.6 (9.1, 10.0)	9.6 (9.2, 10.1)	10.3 (9.4, 11.2)

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the CORAIL/Trabecular Metal (Shell) total conventional hip combination is compared to all other total conventional hip prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Conventional Hip Replacement

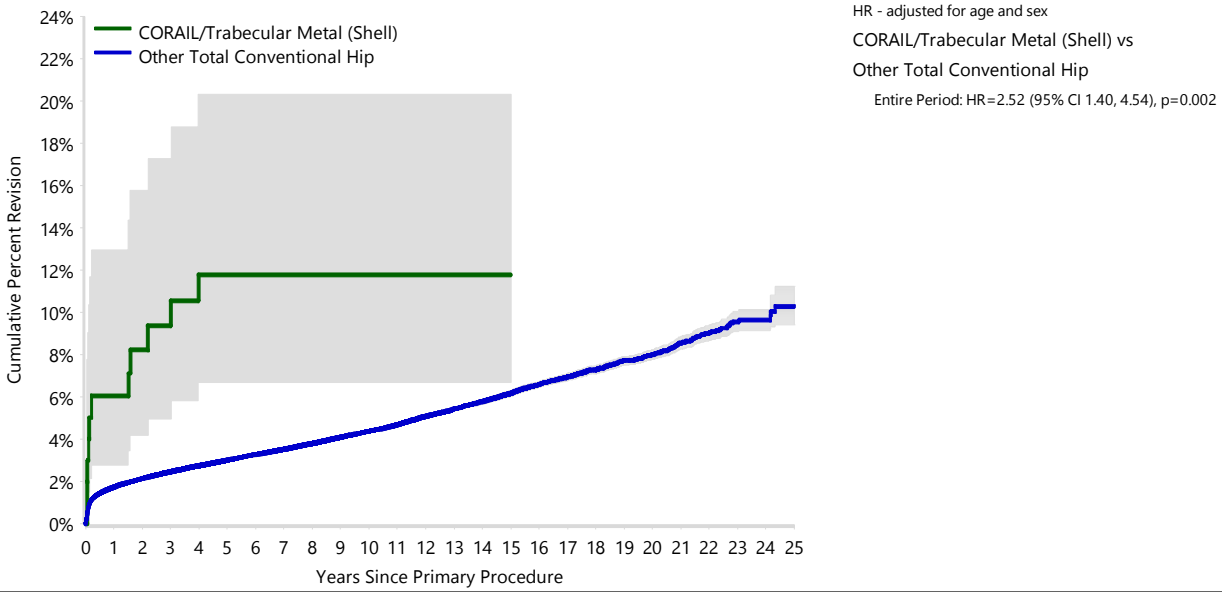

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs
CORAIL/Trabecular Metal (Shell)	100	89	80	77	72	70	68	66
Other Total Conventional Hip	568512	501514	445353	391487	344317	299284	259448	220882

Number at Risk	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
CORAIL/Trabecular Metal (Shell)	61	57	52	47	41	33	25	20	9
Other Total Conventional Hip	185737	153682	124796	99528	79761	63310	49705	38013	28346

Number at Risk	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	24 Yrs	25 Yrs
CORAIL/Trabecular Metal (Shell)	5	2	0	0	0	0	0	0	0
Other Total Conventional Hip	20432	14636	10400	7396	4859	2863	1455	560	95

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 3

Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total conventional hip prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

	CORAIL/Trabecular Metal (Shell)		Other Total Conventional Hip	
Primary Diagnosis	Number	Percent	Number	Percent
Osteoarthritis	7	63.6	16289	82.7
Fractured Neck Of Femur	1	9.1	1520	7.7
Osteonecrosis	1	9.1	843	4.3
Developmental Dysplasia			321	1.6
Rheumatoid Arthritis			201	1.0
Failed Internal Fixation			165	0.8
Tumour			157	0.8
Other Inflammatory Arthritis			102	0.5
Fracture/Dislocation	2	18.2	58	0.3
Other			21	0.1
Arthrodesis Takedown			13	0.1
TOTAL	**11**	**100.0**	**19690**	**100.0**

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Conventional Hip Replacement - Reason for Revision (Follow-up Limited to 18.6 Years)

	CORAIL/Trabecular Metal (Shell)			Other Total Conventional Hip		
Revision Diagnosis	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	4	4.0	36.4	4997	0.9	25.5
Prosthesis Dislocation/Instability	2	2.0	18.2	4369	0.8	22.3
Fracture	1	1.0	9.1	4326	0.8	22.1
Loosening	4	4.0	36.4	3594	0.6	18.4
Pain				338	0.1	1.7
Leg Length Discrepancy				307	0.1	1.6
Malposition				281	0.0	1.4
Implant Breakage Stem				207	0.0	1.1
Lysis				191	0.0	1.0
Implant Breakage Acetabular Insert				126	0.0	0.6
Wear Acetabular Insert				100	0.0	0.5
Incorrect Sizing				96	0.0	0.5
Metal Related Pathology				88	0.0	0.4
Implant Breakage Acetabular				71	0.0	0.4
Wear Head				47	0.0	0.2
Tumour				46	0.0	0.2
Heterotopic Bone				26	0.0	0.1
Implant Breakage Head				25	0.0	0.1
Wear Acetabulum				6	0.0	0.0
Osteonecrosis				4	0.0	0.0
Synovitis				2	0.0	0.0
Progression Of Disease				1	0.0	0.0
Other				320	0.1	1.6
N Revision	**11**	**11.0**	**100.0**	**19568**	**3.4**	**100.0**
N Primary	**100**			**568512**		

Note: This table is restricted to revisions within 18.6 years for all groups to allow a time-matched comparison of revisions.
Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Conventional Hip Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the CORAIL/Trabecular Metal (Shell) total conventional hip combination. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total conventional hip prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Conventional Hip Replacement

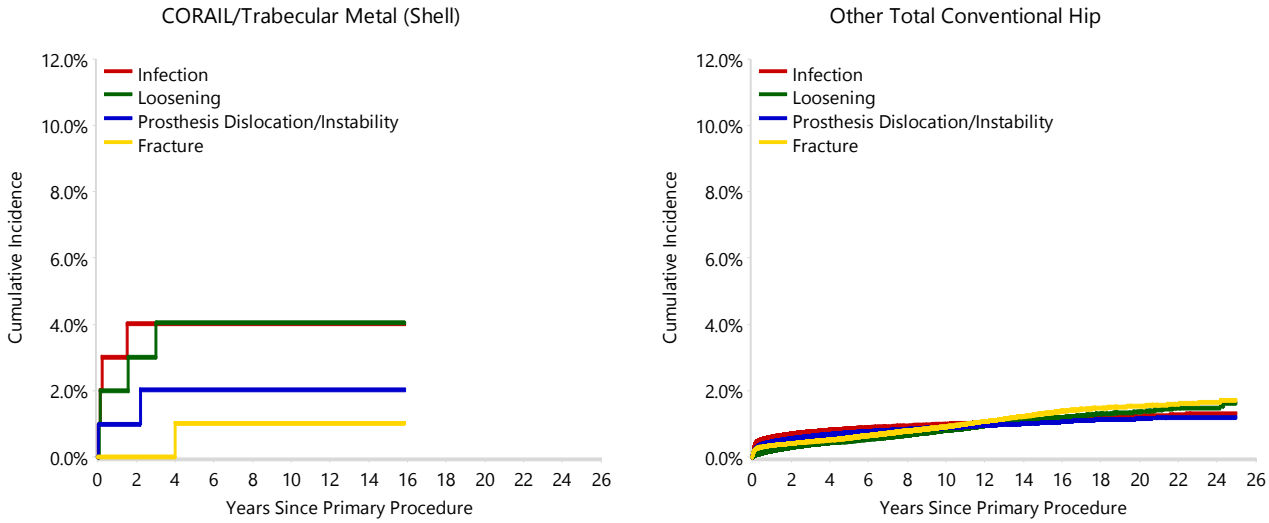

TABLE 5

Type of Revision Performed for Primary Total Conventional Hip Replacement

This analysis identifies the components used in the revision of the CORAIL/Trabecular Metal (Shell) total conventional hip combination and compares it to the components used in the revision of all other total conventional hip prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total conventional hip prostheses i.e. is there a difference in the type of revision undertaken for the CORAIL/Trabecular Metal (Shell) total conventional hip combination compared to all other total conventional hip prostheses.

Table 5: Primary Total Conventional Hip Replacement - Type of Revision (Follow-up Limited to 18.6 Years)

	CORAIL/Trabecular Metal (Shell)		Other Total Conventional Hip	
Type of Revision	Number	Percent	Number	Percent
Femoral Component	3	27.3	6616	33.8
Acetabular Component	2	18.2	3276	16.7
THR (Femoral/Acetabular)	1	9.1	2275	11.6
Cement Spacer			556	2.8
Removal of Prostheses	1	9.1	91	0.5
Reinsertion of Components			27	0.1
Total Femoral			12	0.1
Bipolar Head and Femoral			10	0.1
N Major	**7**	**63.6**	**12863**	**65.7**
Head/Insert	2	18.2	5340	27.3
Head Only			911	4.7
Minor Components	1	9.1	284	1.5
Insert Only	1	9.1	167	0.9
Bipolar Only			1	0.0
Cement Only			1	0.0
Head/Neck/Insert			1	0.0
N Minor	**4**	**36.4**	**6705**	**34.3**
TOTAL	**11**	**100.0**	**19568**	**100.0**

Note: This table is restricted to revisions within 18.6 years for all groups to allow a time-matched comparison of revisions.
Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 6

Revision Rates of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Fixation

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Fixation

Fixation	N Revised	N Total
Cementless	10	86
Hybrid (Femur Cemented)	0	1
Reverse Hybrid (Femur Cementless)	1	13
TOTAL	**11**	**100**

TABLE 7

Revision Rates of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Bearing Surface

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this combination are listed.

Table 7: Revised Number of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Ceramic/Non XLPE	0	1
Ceramic/XLPE	4	31
Ceramic/XLPE + Antioxidant	0	1
Metal/Non XLPE	1	3
Metal/XLPE	6	64
TOTAL	**11**	**100**

TABLE 8

Revision Rates of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Approach

This analysis is provided as some prostheses are used with a variety of surgical approaches. All surgical approaches used with this combination are listed.

Table 8: Revised Number of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Approach

Approach	N Revised	N Total
Lateral	1	6
Posterior	1	11
TOTAL	**2**	**17**

Note: Excludes 83 procedures with no approach recorded

TABLE 9

Revision Rates of Primary Total Conventional Hip Replacement by State

This enables a state by state variation to be identified for the CORAIL/Trabecular Metal (Shell) total conventional hip combination and provides the comparative data for each of the states for all other total conventional hip prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 9: Revised Number of Primary Total Conventional Hip Replacement by State

Component	State	N Revised	N Total
CORAIL/Trabecular Metal (Shell)	NSW	0	3
	VIC	6	34
	QLD	1	27
	WA	3	30
	SA	0	2
	TAS	1	4
Other Total Conventional Hip	NSW	5507	166999
	VIC	4847	146524
	QLD	3967	104332
	WA	2507	64916
	SA	1887	52082
	TAS	438	18265
	ACT/NT	537	15394
TOTAL		**19701**	**568612**

Note: Prostheses no longer used in 2025 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 10

Number of Revisions of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Year of Implant

This analysis details the number of prostheses reported each year to the Registry for the CORAIL/Trabecular Metal (Shell) total conventional hip combination. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2025 has a maximum of one year to be revised, whereas a primary procedure performed in 2023 has a maximum of three years to be revised.

Table 10: Number of Revisions of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2007	2	5
2008	3	10
2009	1	17
2010	2	20
2011	0	9
2012	1	8
2013	0	8
2014	0	6
2015	0	1
2016	2	6
2017	0	2
2018	0	4
2019	0	1
2020	0	1
2024	0	1
2025	0	1
TOTAL	**11**	**100**

TABLE 11

Revision Rates of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular CORAIL/Trabecular Metal (Shell) prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Material	Coating	Fixation
Femoral Stem						
CORAIL	3L92498-3L92521	STANDARD CEMENTLESS FEMORAL STEM W/COLLAR	NO	METAL	HA COATED	
CORAIL	3L92507-3L92520	STANDARD CEMENTLESS FEMORAL STEM W/OUT COLLAR	NO	METAL	HA COATED	
CORAIL	3L93709-3L93720	CEMENTLESS LATERALISED FEMORAL STEM W/COLLAR	NO	METAL	HA COATED	
CORAIL	L20309-L20320	CEMENTLESS HIGH OFFSET FEMORAL STEM W/OUT COLLAR	NO	METAL	HA COATED	
CORAIL	L971109-L971120	CEMENTLESS FEMORAL STEM HIGH OFFSET COLLAR	NO	METAL		
Acetabular						
Trabecular Metal (Shell)	00620203820-00620208020	TRABECULAR METAL MODULAR ACETABULAR SHELL WITH MULTI HOLES POROUS TIVANIUM/TANTALUM	NO	METAL		HIGHLY POROUS
Trabecular Metal (Shell)	00620203822-00620208022	TRABECULAR METAL MODULAR ACETABULAR SHELL WITH CLUSTER HOLES POROUS TIVANIUM/TANTALUM	NO	METAL		HIGHLY POROUS
Trabecular Metal (Shell)	00700004820-00700008070	TRABECULAR METAL ACETABULAR REVISION SHELL TANTALUM/TITANIUM ALLOY	NO	METAL		HIGHLY POROUS

Table 11: Revised Number of CORAIL/Trabecular Metal (Shell) Primary Total Conventional Hip Replacement by Catalogue Number Range

Femoral Stem Range	Acetabular Range	N Revised	N Total
3L92498-3L92521	00620203820-00620208020	1	8
	00620203822-00620208022	0	15
	00700004820-00700008070	0	2
3L92507-3L92520	00620203820-00620208020	2	17
	00620203822-00620208022	3	19
	00700004820-00700008070	1	2
3L93709-3L93720	00620203820-00620208020	2	7
	00620203822-00620208022	0	16
	00700004820-00700008070	0	2
L20309-L20320	00620203820-00620208020	2	8
	00620203822-00620208022	0	1
	00700004820-00700008070	0	1
L971109-L971120	00620203820-00620208020	0	1
	00700004820-00700008070	0	1

Femoral Stem Range	Acetabular Range	N Revised	N Total
TOTAL		11	100