

Trekking/Trekking Total Knee Investigation

Note: This analysis compares the Trekking/Trekking femoral/tibial combination with all other total knee prostheses.

This combination has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2026>.

Note: Procedures using prostheses with no recorded use in 2025 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Knee Replacement

The revision rate of the Trekking/Trekking total knee combination is compared to all other total knee prostheses.

Table 1: Revision Rates of Primary Total Knee Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
Trekking/Trekking	83	1311	11383	0.73 (0.58, 0.90)
Other Total Knee	27201	790119	5134539	0.53 (0.52, 0.54)
TOTAL	27284	791430	5145922	0.53 (0.52, 0.54)

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Trekking/Trekking total knee combination is compared to all other total knee prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Knee Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs
Trekking/Trekking	2.2 (1.5, 3.2)	3.3 (2.5, 4.4)	4.0 (3.1, 5.2)	4.7 (3.6, 6.0)	4.9 (3.9, 6.2)	5.7 (4.5, 7.1)
Other Total Knee	1.0 (1.0, 1.0)	1.8 (1.8, 1.8)	2.4 (2.3, 2.4)	2.8 (2.7, 2.8)	3.1 (3.0, 3.1)	3.4 (3.4, 3.5)

CPR	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs
Trekking/Trekking	6.0 (4.8, 7.4)	6.2 (5.0, 7.7)	6.5 (5.2, 8.1)	6.5 (5.2, 8.1)	6.9 (5.6, 8.6)	7.2 (5.8, 9.1)
Other Total Knee	3.7 (3.7, 3.8)	4.0 (4.0, 4.1)	4.3 (4.3, 4.4)	4.6 (4.6, 4.7)	4.9 (4.9, 5.0)	5.3 (5.2, 5.3)

CPR	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs
Trekking/Trekking	7.7 (6.1, 9.9)	7.7 (6.1, 9.9)				
Other Total Knee	5.6 (5.5, 5.7)	5.9 (5.8, 6.0)	6.3 (6.2, 6.4)	6.7 (6.6, 6.9)	7.2 (7.0, 7.3)	7.5 (7.4, 7.7)

CPR	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	24 Yrs	25 Yrs
Trekking/Trekking							
Other Total Knee	7.8 (7.7, 8.0)	8.1 (7.9, 8.3)	8.5 (8.2, 8.7)	8.7 (8.4, 9.0)	8.8 (8.5, 9.1)	9.1 (8.7, 9.5)	9.5 (8.8, 10.2)

Note: Prostheses no longer used in 2025 are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Trekking/Trekking total knee combination is compared to all other total knee prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Knee Replacement

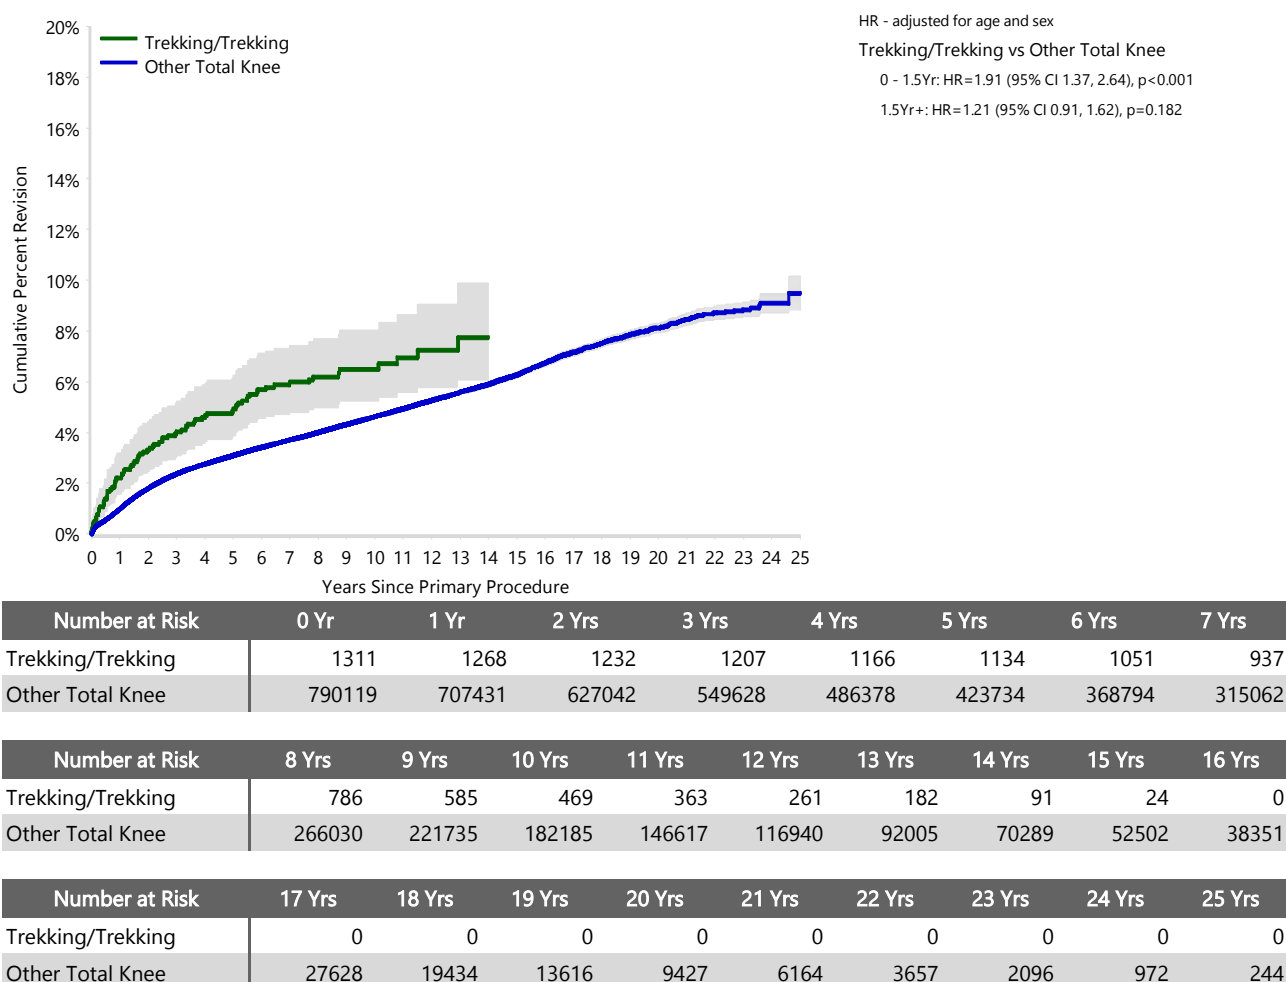

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 3

Primary Diagnosis for Revised Primary Total Knee Replacement

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total knee prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Knee Replacement

Primary Diagnosis	Trekking/Trekking		Other Total Knee	
	Number	Percent	Number	Percent
Osteoarthritis	80	96.4	26312	96.7
Rheumatoid Arthritis			330	1.2
Tumour			199	0.7
Other Inflammatory Arthritis	3	3.6	174	0.6
Osteonecrosis			104	0.4
Fracture			55	0.2
Other			26	0.1
Chondrocalcinosis			1	0.0
TOTAL	83	100.0	27201	100.0

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Knee Replacement - Reason for Revision (Follow-up Limited to 15.5 Years)

Revision Diagnosis	Trekking/Trekking			Other Total Knee		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	19	1.4	22.9	7806	1.0	29.2
Loosening	29	2.2	34.9	5619	0.7	21.0
Instability	7	0.5	8.4	2828	0.4	10.6
Patella Erosion	5	0.4	6.0	1965	0.2	7.4
Pain	2	0.2	2.4	1842	0.2	6.9
Patellofemoral Pain	4	0.3	4.8	1534	0.2	5.7
Arthrofibrosis	4	0.3	4.8	1177	0.1	4.4
Fracture	6	0.5	7.2	1089	0.1	4.1
Malalignment				511	0.1	1.9
Wear Tibial Insert	1	0.1	1.2	338	0.0	1.3
Lysis	1	0.1	1.2	273	0.0	1.0
Implant Breakage Tibial Insert	1	0.1	1.2	222	0.0	0.8
Incorrect Sizing	2	0.2	2.4	215	0.0	0.8
Patella Maltracking				191	0.0	0.7
Bearing Dislocation				148	0.0	0.6
Implant Breakage Patella				145	0.0	0.5
Metal Related Pathology				113	0.0	0.4
Prosthesis Dislocation				78	0.0	0.3
Synovitis				64	0.0	0.2
Osteonecrosis	1	0.1	1.2	50	0.0	0.2
Wear Patella				49	0.0	0.2
Implant Breakage Femoral				45	0.0	0.2
Implant Breakage Tibial				38	0.0	0.1
Tumour				36	0.0	0.1
Heterotopic Bone				16	0.0	0.1
Progression Of Disease				8	0.0	0.0
Wear Tibial				5	0.0	0.0
Patella Dislocation				3	0.0	0.0
Incorrect Side				1	0.0	0.0
Wear Femoral				1	0.0	0.0
Other	1	0.1	1.2	311	0.0	1.2
N Revision	83	6.3	100.0	26721	3.4	100.0
N Primary	1311			790119		

Note: This table is restricted to revisions within 15.5 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2025 are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Knee Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the Trekking/Trekking total knee combination. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total knee prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Knee Replacement

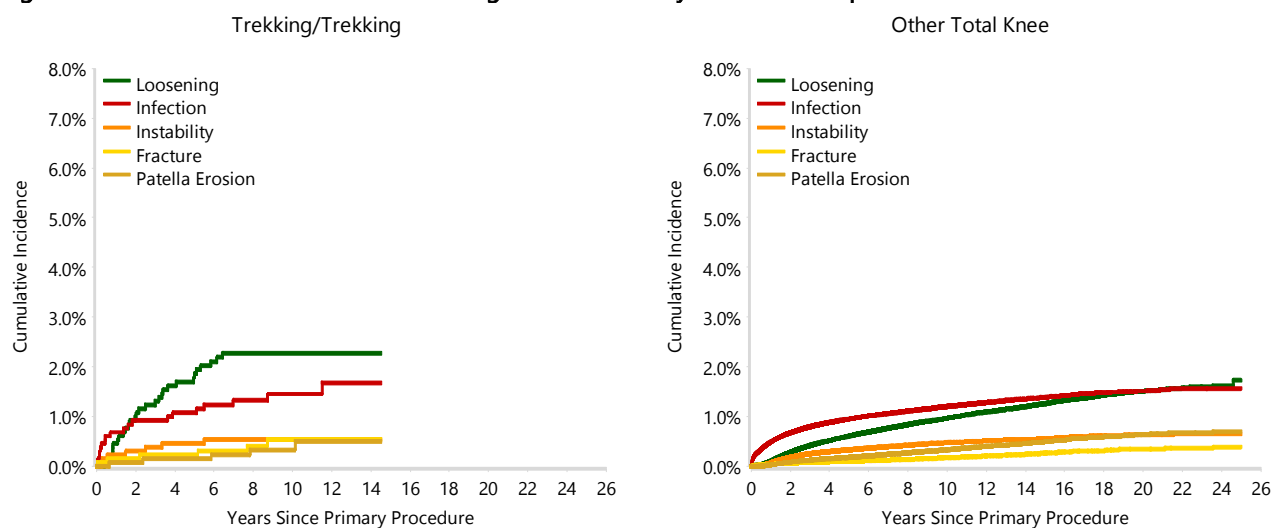


TABLE 5

Type of Revision Performed for Primary Total Knee Replacement

This analysis identifies the components used in the revision of the Trekking/Trekking total knee combination and compares it to the components used in the revision of all other total knee prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total knee prostheses i.e. is there a difference in the type of revision undertaken for the Trekking/Trekking total knee combination compared to all other total knee prostheses.

Table 5: Primary Total Knee Replacement - Type of Revision (Follow-up Limited to 15.5 Years)

Type of Revision	Trekking/Trekking		Other Total Knee	
	Number	Percent	Number	Percent
TKR (Tibial/Femoral)	38	45.8	6452	24.1
Tibial Component	3	3.6	1899	7.1
Femoral Component	8	9.6	1300	4.9
Cement Spacer	4	4.8	1122	4.2
Removal of Prostheses	1	1.2	131	0.5
Total Femoral			21	0.1
Reinsertion of Components			8	0.0
N Major	54	65.1	10933	40.9
Insert Only	13	15.7	8470	31.7
Patella Only	11	13.3	4441	16.6
Insert/Patella	5	6.0	2802	10.5
Minor Components			65	0.2
Cement Only			10	0.0
N Minor	29	34.9	15788	59.1
TOTAL	83	100.0	26721	100.0

Note: This table is restricted to revisions within 15.5 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 6**Revision Rates of Trekking/Trekking Primary Total Knee Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of Trekking/Trekking Primary Total Knee Replacement by Fixation

Fixation	N Revised	N Total
Cemented	34	436
Cementless	22	311
Hybrid (Tibial Cemented)	26	559
Hybrid (Tibial Cementless)	1	5
TOTAL	83	1311

TABLE 7**Revision Rates of Trekking/Trekking Primary Total Knee Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this combination are listed.

Table 7: Revised Number of Trekking/Trekking Primary Total Knee Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Non XLPE	77	1239
XLPE + Antioxidant	6	72
TOTAL	83	1311

TABLE 8**Revision Rates of Trekking/Trekking Primary Total Knee Replacement by Bearing Mobility**

This analysis is provided as some prostheses are combined with a variety of bearing mobilities. All bearing mobilities used with this combination are listed.

Table 8: Revised Number of Trekking/Trekking Primary Total Knee Replacement by Bearing Mobility

Bearing Mobility	N Revised	N Total
Fixed	22	514
Rotating	61	797
TOTAL	83	1311

TABLE 9**Revision Rates of Trekking/Trekking Primary Total Knee Replacement by Stability**

This analysis is provided as some prostheses are combined with a variety of stabilities. All stabilities used with this combination are listed.

Table 9: Revised Number of Trekking/Trekking Primary Total Knee Replacement by Stability

Stability	N Revised	N Total
Minimally Stabilised	42	839
Posterior Stabilised	41	472
TOTAL	83	1311

TABLE 10

Revision Rates of Primary Total Knee Replacement by State

This enables a state by state variation to be identified for the Trekking/Trekking total knee combination and provides the comparative data for each of the states for all other total knee prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 10: Revised Number of Primary Total Knee Replacement by State

Component	State	N Revised	N Total
Trekking/Trekking	NSW	16	105
	VIC	34	408
	QLD	17	463
	WA	4	58
	TAS	3	19
	ACT/NT	9	258
Other Total Knee	NSW	7534	259392
	VIC	5986	163157
	QLD	5772	166781
	WA	3596	92783
	SA	3220	73114
	TAS	472	15056
	ACT/NT	621	19836
TOTAL		27284	791430

Note: Prostheses no longer used in 2025 are excluded from the comparator.

TABLE 11**Number of Revisions of Trekking/Trekking Primary Total Knee Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the Trekking/Trekking total knee combination. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2025 has a maximum of one year to be revised, whereas a primary procedure performed in 2023 has a maximum of three years to be revised.

Table 11: Number of Revisions of Trekking/Trekking Primary Total Knee Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2010	5	35
2011	7	102
2012	13	133
2013	8	107
2014	4	108
2015	3	106
2016	9	129
2017	13	216
2018	7	143
2019	8	100
2020	4	65
2021	0	20
2022	2	18
2023	0	10
2024	0	12
2025	0	7
TOTAL	83	1311

TABLE 12

Revision Rates of Trekking/Trekking Primary Total Knee Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular Trekking/Trekking prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Coating
Femoral				
Trekking	GSP0001-GSP0105	FEMORAL COMPONENT CR	YES	
Trekking	GSP0001P-GSP0105P	CR PRESSFIT FEMORAL	NO	HA COATED
Trekking	GSP0002N-GSP0002N	FEMORAL COMPONENT CR	YES	
Trekking	GSP0004PN-GSP0104PN	CR PRESSFIT FEMORAL	NO	HA COATED
Trekking	GSP1001-GSP1105	FEMORAL COMPONENT PS	YES	
Trekking	GSP1001P-GSP1105P	PS PRESSFIT FEMORAL	NO	HA COATED
Trekking	GSP1004N-GSP1103N	FEMORAL COMPONENT PS	YES	
Tibial				
Trekking	GSP7011-GSP7015	COCRMO MBHOLLOW TIBIAL TRAY	YES	
Trekking	GSP7011P-GSP7015P	COCRMO PRESSFIT TIBIAL	NO	
Trekking	GSP7011PN-GSP7014PN	TIBIAL TRAY MB HOLLOW COCRMO PRESSFIT	NO	
Trekking	GSP7013N-GSP7014N	COCRMO MBHOLLOW TIBIAL TRAY	YES	
Trekking	GSP7041-GSP7045	FB TIBIAL TRAY COCRMO	YES	
Trekking	GSP7041P-GSP7045P	COCRMO PRESSFIT FB TIBIAL	NO	
Trekking	GSP7042N-GSP7043N	FB TIBIAL TRAY COCRMO	YES	

Table 12: Revised Number of Trekking/Trekking Primary Total Knee Replacement by Catalogue Number Range

Femoral Range	Tibial Range	N Revised	N Total
GSP0001-GSP0105	GSP7011-GSP7015	5	50
	GSP7013N-GSP7014N	0	1
	GSP7041-GSP7045	4	60
GSP0001P-GSP0105P	GSP7011-GSP7015	6	105
	GSP7011P-GSP7015P	10	213
	GSP7011PN-GSP7014PN	1	8
	GSP7041-GSP7045	16	393
	GSP7042N-GSP7043N	0	1
GSP0002N-GSP0002N	GSP7042N-GSP7043N	0	1
GSP0004PN-GSP0104PN	GSP7011-GSP7015	0	1
	GSP7011P-GSP7015P	0	4
	GSP7041-GSP7045	0	2
GSP1001-GSP1105	GSP7011-GSP7015	23	278
	GSP7011P-GSP7015P	1	6
	GSP7013N-GSP7014N	0	3
	GSP7041-GSP7045	2	35
	GSP7041P-GSP7045P	0	1
GSP1001P-GSP1105P	GSP7011-GSP7015	4	31
	GSP7011P-GSP7015P	11	95
	GSP7011PN-GSP7014PN	0	1
	GSP7041-GSP7045	0	17
	GSP7041P-GSP7045P	0	1
GSP1004N-GSP1103N	GSP7011-GSP7015	0	3
	GSP7041-GSP7045	0	1
TOTAL		83	1311